

3D AND MULTISPECTRAL IMAGING FOR SUBCUTANEOUS VEINS DETECTION

F. Meriaudeau *, *V. Paquit* ^{*†}, *N. Walter* *, *J. Price* [†] and *K. Tobin* [†]

*Laboratory Le2i, UMR CNRS 5158

University de Bourgogne

12 rue de La Fonderie, 71200 Le Creusot, France.

E-mail : fmeriau@u-bourgogne.fr

[†] Oak Ridge National Laboratory,

.O. Box 2008, Oak Ridge, TN 37831, USA..

ABSTRACT

The first and perhaps most important phase of a surgical procedure is the insertion of an intravenous (IV) catheter. Currently, this is performed manually by trained personnel. In some visions of future operating rooms, however, this process is to be replaced by an automated system. Experiments to determine the best NIR wavelengths to optimize vein contrast for physiological differences such as skin tone and/or the presence of hair on the arm or wrist surface are presented. For illumination our system is composed of a mercury arc lamp coupled to a 10nm band-pass spectrometer. A structured lighting system is also coupled to our multispectral system in order to provide 3D information of the patient arm orientation. Images of each patient arm are acquired under every possible combination of illuminants and the optimal combination of wavelengths for a given subject to maximize vein contrast using linear discriminant analysis is determined.

Index Terms—3D shape acquisition, multispectral imaging, line detection, medical applications.

1. INTRODUCTION

Biomedical imaging techniques based on wave propagation phenomena in biological tissues are commonly used to detect and treat diseases but are also used to image non-invasively organs and biological structures inside the body. Amongst them, optical tomography is a growing imaging technique offering the advantages to be non-invasive, experimentally simple, repeatable and inexpensive. Optical tomography uses light which offers at specific wavelengths a large variety of interaction phenomena, functions of physiological changes at cellular and subcellular levels, and allows retrieving information on biological systems. Over the last decade, publications in the field have reported promising results [1] as well as really surprising images

[2] of human or animal organs, letting us envision the capabilities of biomedical imaging using light. However, in this field only few researches investigate subcutaneous veins visualization and measurement. Using light propagation properties of tissues in the near infrared range of light, Zeman et al. [3] developed and commercialized, via Luminex, a device to locate subcutaneous veins and back project their position on the imaged skin surface for catheter insertion assistance. The device named VeinViewer works well on the average person, but performance can be decreased significantly based on poorly understood relations to various physiological parameters. This technology also provides no estimation of the relative depth or diameter of vessels, which are key factors in selecting the optimal vein [4]. In preliminary research [5], [6] we have described experiments to determine the best near-infrared (NIR) wavelengths to optimize vein contrast for physiological differences such as skin tone and the presence of hair on the arm or wrist surface but we also noticed a correlation between the skin tone and the projection matrix used for classification as well as misclassification of some pixels due to reflection events and skin structure changes. Further investigations on light propagation in biological tissues [7] indicate that imaging the skin under visible to NIR illuminations will provide interesting reflectance spectrum variability that can be used to improve our classification method. In this paper we are presenting an optimization of our localization process by reducing the misclassification rate of pixels using different multispectral projection techniques, a broadband illumination source, and including the influence of the skin surface topography evaluation. The paper is structured as follows: after presenting our acquisition system and its calibration, computational methods and algorithms used for the classification process are introduced, followed by the obtained results. At last a conclusion and future work are discussed.

2. EXPERIMENTAL SET-UP

Our acquisition system (see fig. 1) is composed of a visible to NIR sensitive CMOS video camera, a NIR line generating laser module and a broadband illumination source (Hg arc lamp) associated with a monochromator for illumination wavelength selection. The equipment is controlled by a computer to synchronize illumination selection and image capture. In order to avoid UV radiation injuries to the skin, a high-pass filter at 495nm is inserted between the lamp and the monochromator. The spectral range of study is comprised between 495nm and 945nm by 10nm step, the upper limit being determined by the spectral sensitivity of the camera in the near infrared. A liquid gel light guide is connected on one hand to the output of the illumination source and on the other hand to a two inches wide collimating probe to maintain uniform illumination on the surface of the skin.

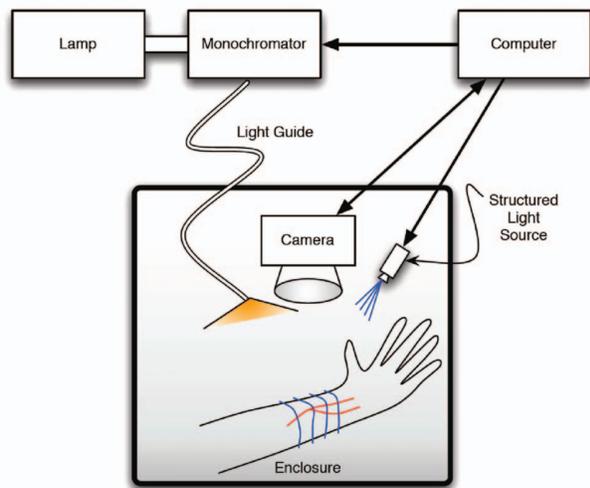


Fig.1 : Experimental set up.

The system calibration consists of three separate steps: (1) image distortion correction by retrieving the optical parameters of the camera [8], (2) reflectance image computation using black and white spectralons as references [9] and (3) parameterization of the triangulation geometry [10]. Fig. 2 presents an example of the obtained images.


3. 3D RECONSTRUCTION

Our 3D reconstruction process of the skin surface combines active optical triangulation for range data acquisition, and parametric surface modeling to store the 3D shape of the


object. Active optical triangulation [10] combines a camera and a laser stripe line generator to recreate a basic geometric system. The camera is aligned along the Z axis and the laser line generator is positioned at a distance b from the camera with the angle θ relative to the X axis. Assuming that the considered laser point coordinates (x,y,z) in the 3D baseline has a projection (u,v) on the image plane, the similar triangles equations gives the mathematical relation between the measured quantities (u,v,θ) and the coordinates (x,y,z) :

$$[x, y, z] = \frac{b}{f \cdot \cot \theta - u} [u, v, f] \quad (1)$$

Parameters b , f and θ are calculated during the system calibration and remain constant during the acquisition phase. In a NIR image of the laser lines on the surface of the skin as on Fig 2.a, the centreline of each line is firstly detected using a sub pixel operator [11], see Fig. 2.b, and secondly triangulated using Equation 1, see Figure 2.c. To simplify the three-dimensional surface modelling of the skin, the triangulated point clouds are associated with a Bezier surface [12]. At the same time the elevation map of the area of interest and the normal to the surface for each pixel using a specific ray tracing algorithm [13] are computed. This data will be used later as a feature in the Linear Discriminant Analysis.

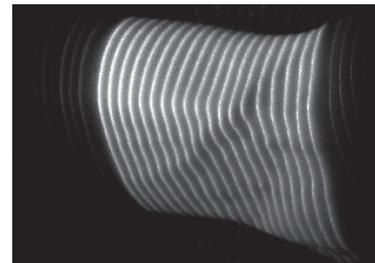

(a)

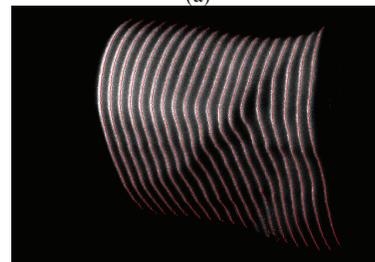

(b)

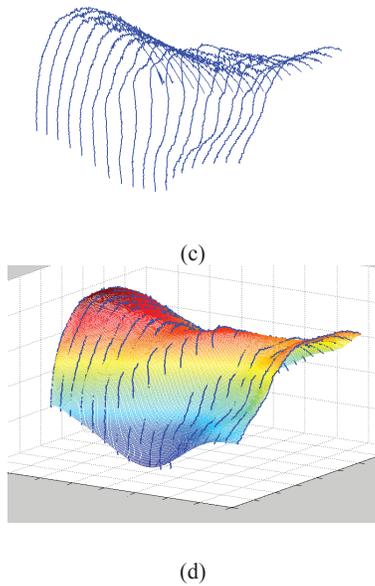


Fig.2 : (a) NIR image of the structured laser lines on the surface of the skin, (b) centerlines detected a subpixel operator are in red, (c) 3D point cloud resulting from triangulation, (d) example of Bézier surface fitting with a (20x20) dimensional Bézier patch.


4. IMAGE PROCESSING AND LINEAR DISCRIMINANT ANALYSIS

Multispectral imaging is commonly used to obtain reflectance measurements of an object in several spectral bands. As a result, each pixel of the image is expected to have specific intensity values over the light spectrum, corresponding to the so called spectral signature. In our experiment, the skin is imaged from 495nm to 945nm by step of 10nm, giving a total of 46 images of the same scene. To analyze this 46-dimensional dataset a multispectral dimension reduction technique, which consists in projecting the initial dataset in a lower dimensional subspace where spectral information is more compact, and less correlated, was used. As aforesaid, our goal is to locate subcutaneous structures for various skin tones. This problem can be seen as a two class classification problem: vein/not-vein or a three class problem vein/skin /background. To reduce our dataset, two well-known linear dimension reduction techniques: Principal Component Analysis [13] and Linear Discriminant Analysis [13] were tried. Then, the resulting image corresponding to the projection of the initial data set onto the subspace spanned by the eigenvector of the first eigenvalue was processed using the Steger's algorithm [14] to detect the veins as well as their respective width. The surface orientation obtained after the triangulation and the normal of the surface is also added to the data set leading to a 47 input feature vectors. For the LDA, which requires a

prior class identification in order to establish the projection matrix, the mask was automatically provided after processing the PCA image [16]. Two labeling masks were used: (a) a two class mask vein / background, and (b) a three class mask vein / skin / background [16].

5. RESULTS

Fig 3. is an example of some of the obtained results after projecting the data by LDA then extracting the veins. The first row corresponds to a two class problem where the mask for the class is manually defined by the operator and serves as a reference. The second row is for the two class problem with mask automatically generated from the PCA image. Third row corresponds to the 3 class problem with manually defined mask. Fourth row corresponds to the three class problem with mask automatically generated from the PCA image.

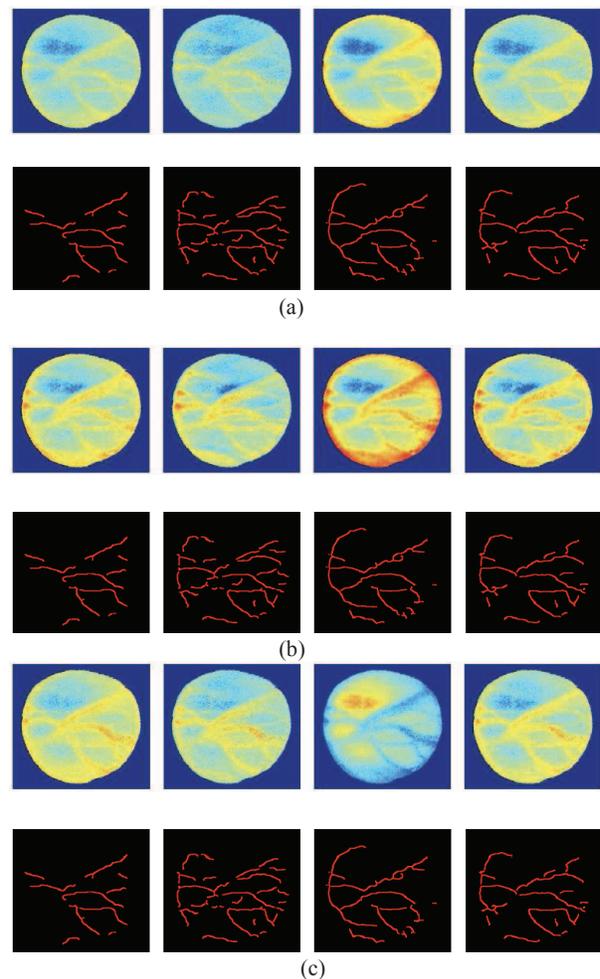

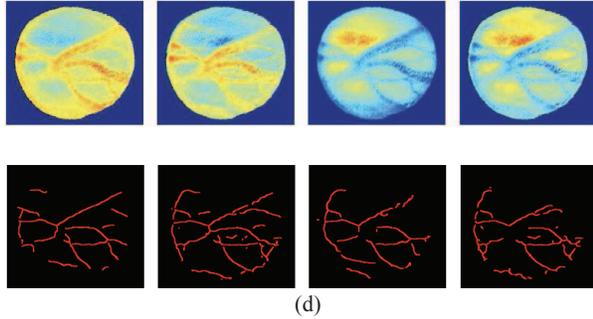


Fig 3: LDA projection and Veins segmentation. From left to right : 2 classes manually defined, 2 classes with mask automatically generated, 3 classes manually defined, 3 classes with mask automatically generated. (a) Only NIR images are projected. (b) NIR images as well as the 3D map are projected. (c) NIR images and visible images are projected. (d) NIR images, visible images and 3D map are projected.

This process was carried out over a panel of 20 patients having different skin tones and different body mass indexes. The results were similar showing that the 2 class problems with mask automatically generated and the input feature set including the 3D information provides results very close to those obtained with the manual mask. We also found out that the projection matrix for a specific skin tone can also be used for another patient of similar skin tone (based on the appearance compared to the Mac Beth chart), however the opposite is not reliable [6].

6. CONCLUSION

We showed in this paper a complete vision system providing multispectral as well as 3D information of the arm surface for automatic veins detection. The LDA projection of the multispectral images in the NIR and visible spectrum associated with 3D information of the arm topography lead to reliable results for automatic veins detection. However our long-term goal being to develop a fully-automated, vision-guided robotic system for needle insertion and catheterization, furthermore examination of the optimal wavelength combinations for different skin tone and/or presence of hair still need further investigation. We are also currently increasing our database to further validate the obtained results.

7. REFERENCES

[1] E. M. C. Hillman, "Experimental and theoretical investigations of near infrared tomographic imaging methods and clinical applications", Ph.D. thesis, University of London, London, UK, (2002).

[2] E. M. Hillman and A. Moore, "All-optical anatomical coregistration for molecular imaging of small animals using dynamic contrast", *Nat Photon*, 1, 9, 526–530, (2007).

[3] H. D. Zeman, G. Lovhoiden, C. Vrancken, and R. K. Danish, "Prototype vein contrast enhancer," *Optical Engineering*, 44, 8, 086401, (2005).

[4] V. C. Paquit, F. Meriaudeau, J. R. Price and K.W. Tobin, *Proceedings of IEEE Conference on EMBC*, Vancouver, (2008).

[5] V. Paquit, J. Price, R. Seulin, F. Meriaudeau, R. Farahi, K. W. Tobin and T.L. Ferrell, "Near-infrared imaging and structured light ranging for automatic catheter insertion," *In proceeding of Medical Imaging , SPIE*, (2006).

[6] V. Paquit, J. Price, F. Meriaudeau, K. Tobin, "Combining near-infrared illuminants to optimize venous imaging," *In proceeding of Medical Imaging Medical Imaging 2007*, SPIE, (2007).

[7] R. R. Anderson et al., "The optics of human skin," *Journal of Investigative Dermatology*, 77, 13-19, (1981).

[8] Z. Zhang, "Flexible Camera Calibration by Viewing a Plane from Unknown Orientations", *In proceeding of ICCV conference*, 666-673, (1999).

[9] Z. Pan et al., "Face recognition in hyperspectral images," *IEEE Transactions on Pattern Analysis and Machine Intelligence*, 25, 12, 1552–1560, (2003).

[10] R.A. Jarvis, "A perspective on range-finding techniques for computer vision," *IEEE Transactions on Pattern Analysis and Machine Intelligence*, 5, 122–139, (1983).

[11] J. Forest, J. M. Teixidor, J. Salvi, and E. Cabruja, "A Proposal for Laser Scanners Sub-pixel Accuracy Peak Detector," *in Workshop on European Scientific and Industrial Collaboration*, 525–532, (Mickolj (Hungria)), May 2003.

[12] P. E. Bézier, "Emploi des machines à commande numérique," *Masson et Cie.*, (1970).

[13] A. Efremov et al., "Robust and numerically stable Bézier clipping method for ray tracing nurbs surfaces", in proceedings of SCCG 2005, 123-131, ACM, (2005).

[14] K. Fukunaga, *Statistical Pattern Recognition*, Morgan Kaufmann, (1990).

[15] Steger, C., "Extraction of curved lines from images", *In 13th International Conference on Pattern Recognition*, 2, 251–255. (1996).

[16] V. Paquit, *Imagerie multispectrale et modélisation 3D pour l'estimation quantitative des vaisseaux sanguins sous cutanés*, Ph.D. thesis, University of Bourgogne, Le Creusot, France, (2008).